

SenTix[®] 51, 52

SenTix[®] 60, 61, 62

SenTix[®] 81, 82

SenTix[®] 91, 92

SenTix[®] Mic, Mic-B, Mic-D

SenTix[®]

PH ELECTRODES WITH LIQUID REFERENCE SYSTEM



a xylem brand

Copyright

© 2016, Xylem Analytics Germany GmbH
Printed in Germany.

Technical data

General data

WTW Model	Reference electrolyte	Junction	NTC	Special features
SenTix® 51	KCl 3 mol/L, Ag ⁺ free	Ceramic	Yes	Plastic shaft
SenTix® 52	KCl 3 mol/L, Ag ⁺ free	Ceramic	Yes	Plastic shaft
SenTix® 60	KCl 3 mol/L, Ag ⁺ free	Platinum	No	
SenTix® 61	KCl 3 mol/L, Ag ⁺ free	Platinum	No	
SenTix® 62	KCl 3 mol/L, Ag ⁺ free	Platinum	No	
SenTix® 81	KCl 3 mol/L, Ag ⁺ free	Platinum	Yes	
SenTix® 82	KCl 3 mol/L, Ag ⁺ free	Platinum	Yes	
SenTix® 91	KCl 3 mol/L, Ag ⁺ free	Platinum	Yes	Longer shaft
SenTix® 92	KCl 3 mol/L, Ag ⁺ free	Platinum	Yes	Longer shaft
SenTix® Mic	KCl 3 mol/L, Ag ⁺ free	Ceramic	No	Half micro combination electrode
SenTix® MIC-B	KCl 3 mol/L, Ag ⁺ free	Platinum	No	Micro combination electrode
SenTix® MIC-D	KCl 3 mol/L, Ag ⁺ free	Platinum	No	Micro combination electrode

Measurement and application characteristics

WTW Model	pH measuring range	Allowed temperature range	Membrane resistance at 25 °C	Typical application
SenTix® 51	0 ... 14	0 ... 80 °C	< 1 GOhm	Field
SenTix® 52	0 ... 14	0 ... 80 °C	< 1 GOhm	Field
SenTix® 60	0 ... 14	0 ... 100 °C	< 600 MOhm	Laboratory
SenTix® 61	0 ... 14	0 ... 100 °C	< 600 MOhm	Laboratory
SenTix® 62	0 ... 14	0 ... 100 °C	< 600 MOhm	Laboratory
SenTix® 81	0 ... 14	0 ... 100 °C	< 600 MOhm	Laboratory
SenTix® 82	0 ... 14	0 ... 100 °C	< 600 MOhm	Laboratory
SenTix® 91	0 ... 14	0 ... 100 °C	< 600 MOhm	Laboratory
SenTix® 92	0 ... 14	0 ... 100 °C	< 600 MOhm	Laboratory
SenTix® Mic	0 ... 14	0 ... 100 °C	< 700 MOhm	Laboratory
SenTix® MIC-B	0 ... 14	-5 ... 100 °C	< 1 GOhm	Laboratory
SenTix® MIC-D	0 ... 14	-5 ... 100 °C	< 1 GOhm	Laboratory

Shaft dimensions, shaft material, electrical connection

WTW Model	Shaft			Electrical connection		
	Length [mm]	Ø [mm]	Material	Electrode connection	Meter connection	Cable length
SenTix® 51	120	12	Polyamide	Fixed cable	DIN*+banana	1 m
SenTix® 52	120	12	Polyamide	Fixed cable	BNC+banana	1 m
SenTix® 60	120	12	Glass	S7 plug-in connector	depending on S7 cable****	
SenTix® 61	120	12	Glass	Fixed cable	DIN*	1 m
SenTix® 62	120	12	Glass	Fixed cable	BNC	1 m
SenTix® 81	120	12	Glass	Fixed cable	DIN*+banana	1 m
SenTix® 82	120	12	Glass	Fixed cable	BNC+banana	1 m
SenTix® 91	170	12	Glass	Fixed cable	DIN*+banana	1 m
SenTix® 92	170	12	Glass	Fixed cable	BNC+banana	1 m
SenTix® Mic	40/80**	12/5**	Glass	S7 plug-in connector	depending on S7 cable****	
SenTix® MIC-B	96***	3	Glass	Fixed cable	BNC	1 m
SenTix® MIC-D	96***	3	Glass	Fixed cable	DIN*	1 m

* Coaxial plug according to DIN 19262

** Stage geometry

*** Measured from upper level of built-in grinding (standard grinding NS 7,5)

**** Connection cable not included in the scope of delivery of the combination electrode (see WEAR PARTS AND ACCESSORIES)


Commissioning, measuring, calibration

Commissioning

The electrode is filled with reference electrolyte solution in the factory. Prepare the electrode for measuring as follows:

- Open the refilling opening for the reference electrolyte solution. Depending on the model, the stopper of the refilling opening is an elastomer stopper or a slider.

The refilling opening must always be open during calibration and measurement!

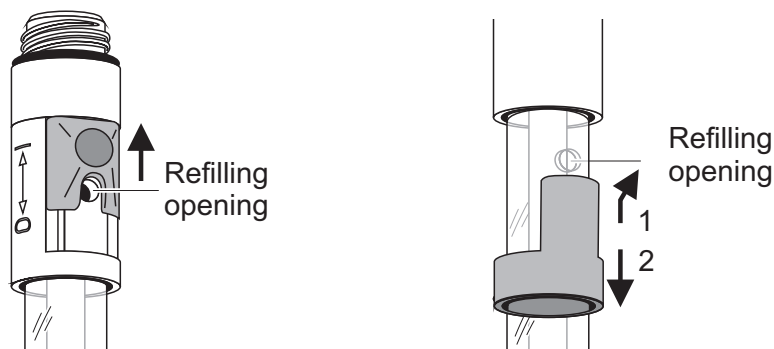

- Remove the watering cap from the electrode tip. Possible salt deposits in


the area of the watering cap do not affect the measuring characteristics and can easily be removed with deionized water.



Please keep the watering cap. It is required for the electrode to be stored. Always keep the watering cap clean.

Calibration and measurement: General rules

- SenTix® 51, SenTix® 52, and SenTix® Mic: Remove any gas bubbles behind the pH membrane by shaking. With all other combination electrodes, gas bubbles behind the pH membrane are not a problem.
- Connect the combination electrode to the meter.
- Calibrate the electrode according to the operating manual of the meter and observe the following rules while doing so:
 - Make sure the refilling opening for the reference electrolyte solution is open.
 - Avoid the displacement of any solution (sample or buffer solution) from one measurement to the next by taking the following measures:
 - Shortly rinse the calibration and sample beakers with the solution the beakers are to be filled with next.
 - Between measurements, rinse the electrode with the solution that follows. Alternatively, you can also rinse the electrode with deionized water and then carefully dab it dry.
 - Immerse the electrode in the solution in a vertical or slightly tilted position.
 - Make sure the immersion depth is correct. The junction must be completely submerged in the solution. The junction is in the area of the bottom end of the shaft (see figure). At the same time, the level of the reference electrolyte must be at least 2 cm above the level of the solution.

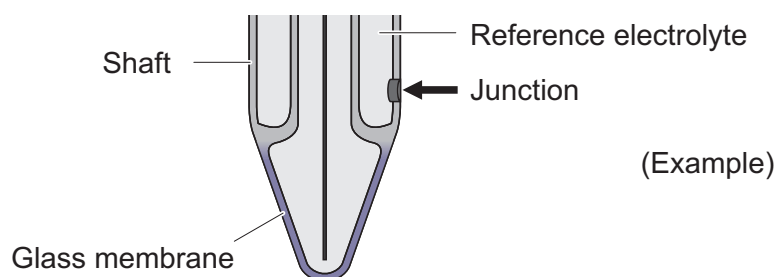

- Provide approximately the same stirring conditions for measuring as for calibrating.



Prevent contact of the pH membrane to the beaker bottom to avoid scratches on the pH membrane.

Subsequent calibrations

The frequency of subsequent calibrations depends on the application. Many meters provide an option where you can enter a calibration interval. After the calibration interval has expired, the meter will automatically remind you of the

due calibration.

Storage

During short measuring breaks

With the refilling opening open, immerse the electrode in reference electrolyte (KCl 3 mol/L, Ag⁺ free). Prior to the next measurement, shortly rinse the electrode with the test sample or deionized water.



Prevent contact of the pH membrane to the beaker bottom to avoid scratches on the pH membrane.

Overnight or longer

Put the clean electrode in the watering cap that is filled with reference electrolyte (KCl 3 mol/L, Ag⁺ free) and close the refilling opening.

NOTE

pH electrodes must not be stored dry or in deionized water. The electrode could be permanently damaged by this. If the liquid in the watering cap has dried up, condition the electrode in reference electrolyte (KCl 3 mol/L, Ag⁺ + free) for at least 24 hours.



During longer storing periods, salt sediments may develop on the watering cap. They do not affect the measuring characteristics and can easily be removed with deionized water when the electrode is put into operation again.

Aging

pH electrodes are consumables. Every pH electrode undergoes a natural aging process. With aging, the responding behavior becomes slower and the electrode slope and asymmetry change. Moreover, extreme operating conditions can considerably shorten the lifetime of the electrode. These are:

- Strong acids or lyes, hydrofluoric acid, organic solvents, oils, fats, bromides, sulfides, iodides, proteins
- High temperatures
- High changes in pH and temperature.


The warranty does not cover failure caused by measuring conditions and mechanical damage.

Maintenance and cleaning

Refilling the reference electrolyte

During operation, a small amount of reference electrolyte leaks through the junction from the electrode into the test sample. If the level of reference electrolyte becomes too low with time, refill it through the refilling opening. Refilling is very easy with the enclosed dropping bottle. Proceed as follows:

- Cut off the tip of the dropping bottle at a right angle until the opening in the tip can be seen
- Open the refilling opening of the electrode
- Press the tip of the dropping bottle into the refilling opening while turning it slightly
- Pump the reference electrolyte in the shaft using the dropping bottle
- Pull the dropping bottle out of the refilling opening while turning it slightly if necessary.

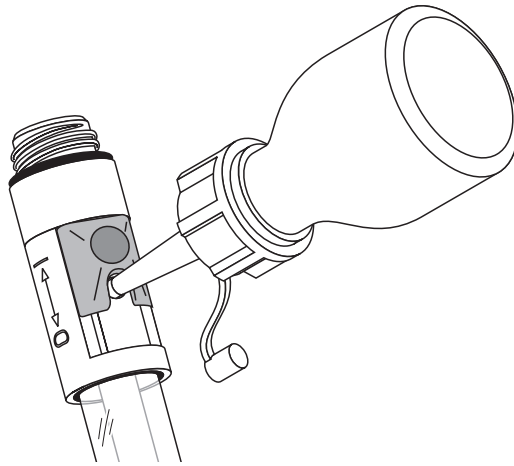

Cleaning Remove water-soluble contamination by rinsing with deionized water. Remove other contamination as follows:

Contamination	Cleaning procedure
Fat and oil	Rinse with water containing household washing-up liquid
Lime and hydroxide deposits	Rinse with citric acid (10 % by weight)
Proteins	Immerse in pepsin cleaning solution PEP/pH for approx. 1 hour. <u>Note:</u> Make sure the level of the reference electrolyte is above that of the cleaning solution.




Hydrofluoric acid, hot phosphoric acid and strong alkaline solutions destroy the glass membrane.

After cleaning

Rinse the electrode with deionized water and condition it in reference electrolyte solution for at least 1 hour. Then recalibrate the electrode.

Wear parts and accessories

Description	Model	Order no.
Reference electrolyte solution 250 mL (KCl 3 mol/L, Ag ⁺ free)	KCl-250	109 705
Plastic arming for SenTix® pH electrodes	A pHLab/K	903 841
Pepsin cleaning solution 3 x 250 ml	PEP/pH	109 648
Connection cable S7 plug-in connector/DIN, 1 m	AS/DIN	108 110
Connection cable S7 plug-in connector/DIN, 3 m	AS/DIN-3	108 112
Connection cable S7 plug-in connector/BNC, 1 m	AS/BNC	108 114



Note

Detailed information on our wide range of buffer solutions and more accessories is given in the price list of the WTW catalog "Laboratory and field instrumentation".

Disposal

At the end of its operational lifetime, the electrode must be returned to the

disposal or return system statutory in your country (electronic waste). If you have any questions, please contact your supplier.

Xylem |'zīləm|

- 1) The tissue in plants that brings water upward from the roots;
- 2) a leading global water technology company.

We're a global team unified in a common purpose: creating advanced technology solutions to the world's water challenges. Developing new technologies that will improve the way water is used, conserved, and re-used in the future is central to our work. Our products and services move, treat, analyze, monitor and return water to the environment, in public utility, industrial, residential and commercial building services settings. Xylem also provides a leading portfolio of smart metering, network technologies and advanced analytics solutions for water, electric and gas utilities. In more than 150 countries, we have strong, long-standing relationships with customers who know us for our powerful combination of leading product brands and applications expertise with a strong focus on developing comprehensive, sustainable solutions.

For more information on how Xylem can help you, go to www.xylem.com.



Service and Returns:

Xylem Analytics Germany
Sales GmbH & Co. KG
WTW
Am Achalaich 11
82362 Weilheim
Germany

Tel.: +49 881 183-325
Fax: +49 881 183-414
E-Mail wtw.rma@xylem.com
Internet: www.xylemanalytics.com

xylem
Let's Solve Water

Xylem Analytics Germany GmbH
Am Achalaich 11
82362 Weilheim
Germany

